

SUPERVISOR TEST

UTICA CITY
 POLICE DEPT
 DATAMASTER dmt: 100282



Date: 11/18/2021

RMS
21-45297

OPERATOR NAME:
 CHRISTOPHER S JENNINGS
 Permit #: 32846
 Operator Agency/Dept: UTICA CITY PD
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:45
INTERNAL STANDARD	VERIFIED	09:45
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.10	09:45
BLANK TEST	0.00	09:46
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:46
BLANK TEST	0.00	09:47
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:48
BLANK TEST	0.00	09:48

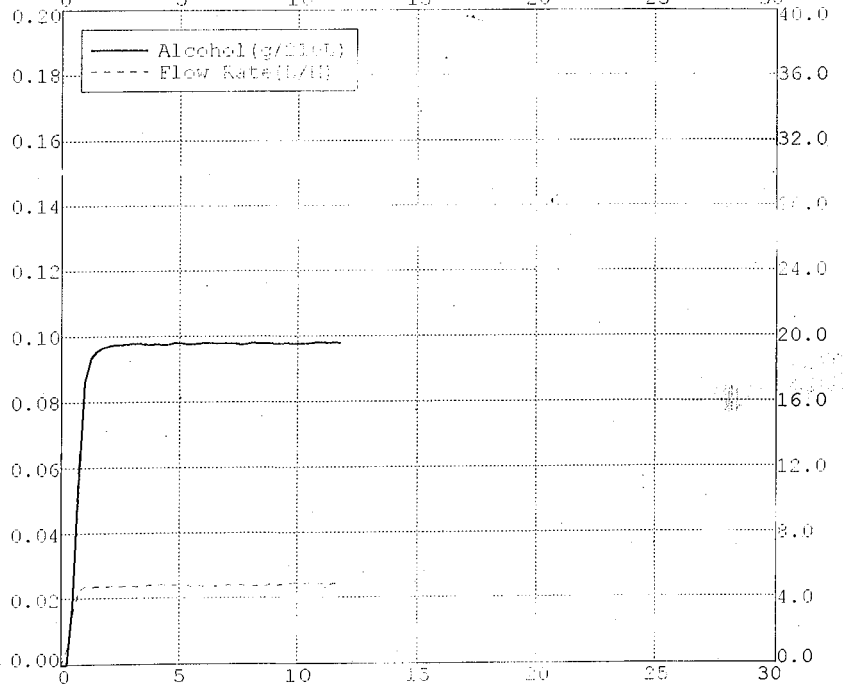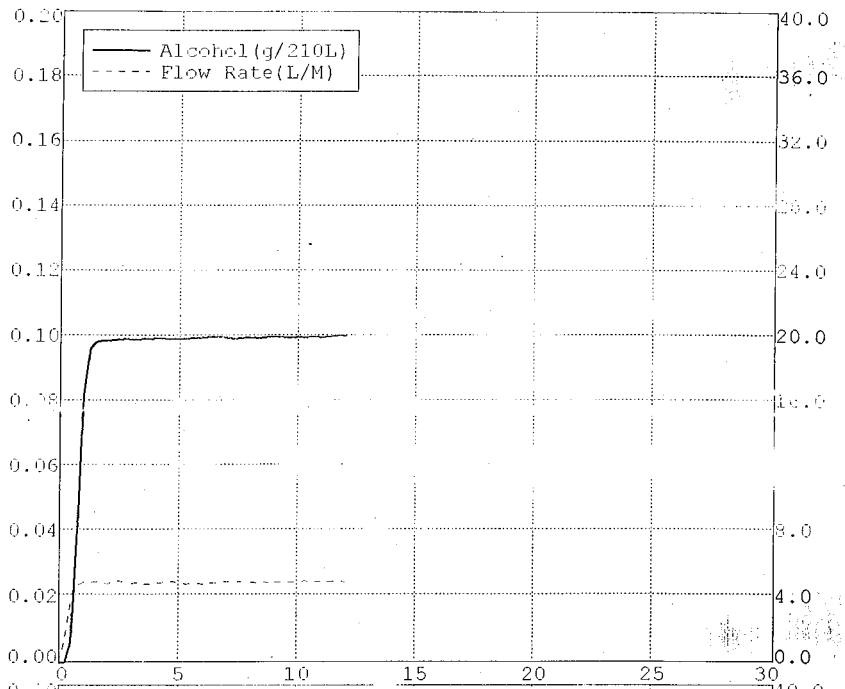

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 11/16/2021

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 21280

RMS
21-45297

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:20
INTERNAL STANDARD	ERROR	15:20

Internal Standard Error