

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 02/19/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:04
INTERNAL STANDARD	VERIFIED	08:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:04
BLANK TEST	0.00	08:05
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:05
BLANK TEST	0.00	08:06
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	08:07
BLANK TEST	0.00	08:07

26-7100

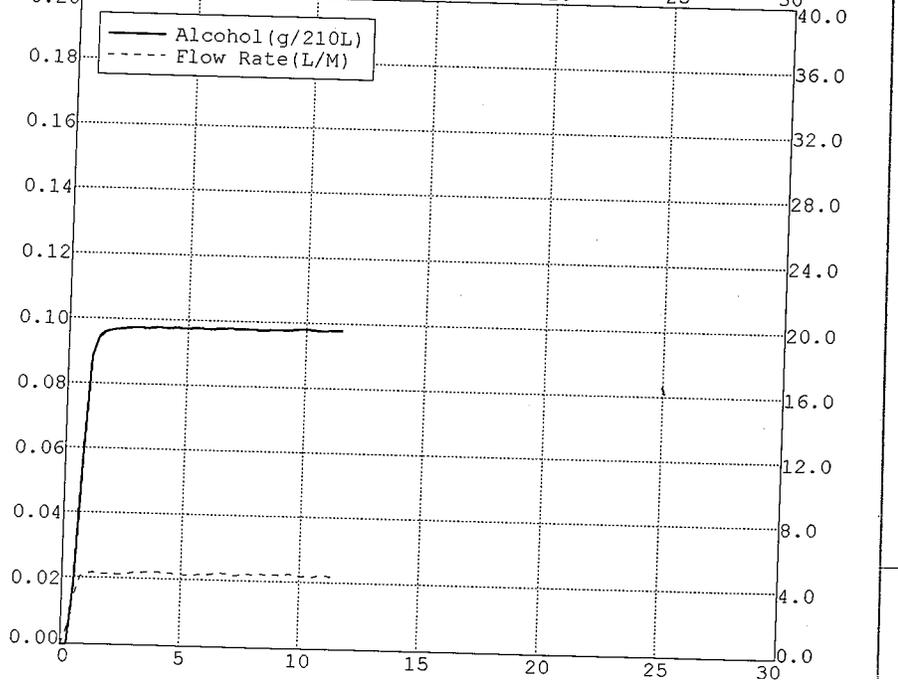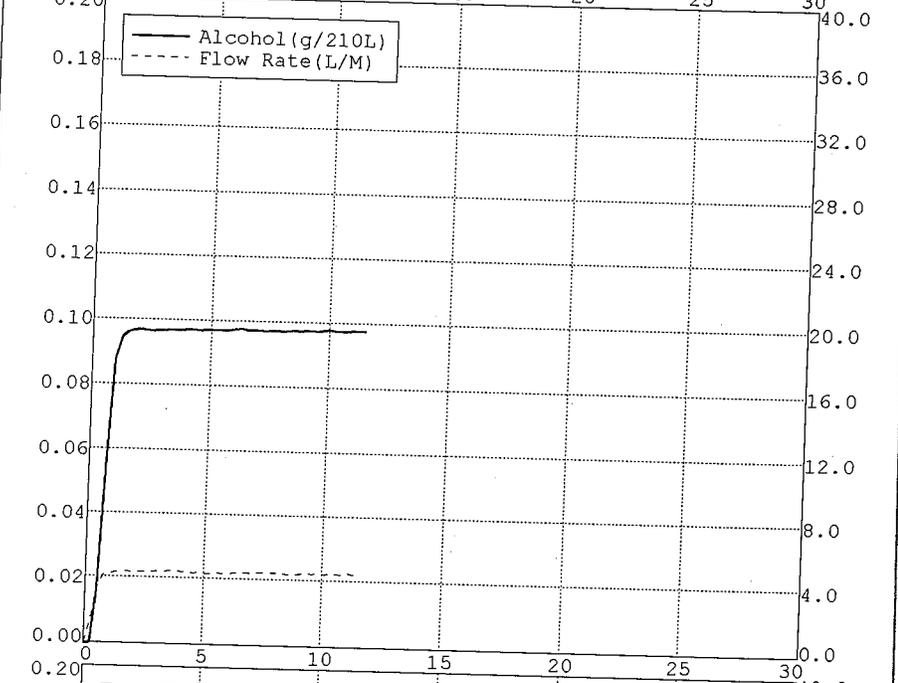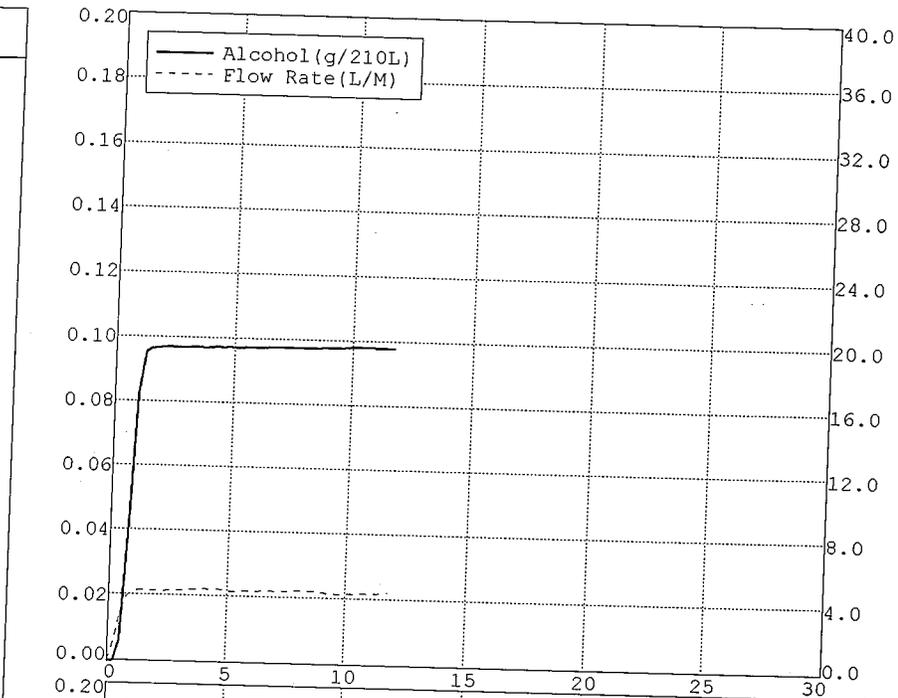

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 02/19/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:57
INTERNAL STANDARD	VERIFIED	07:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:57
BLANK TEST	0.00	07:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:58
BLANK TEST	0.00	07:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	07:59
BLANK TEST	0.00	08:00

26-7100

