

SOLUTION CHANGE

-----  
UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308  
-----




Date: 03/03/2026

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:47
INTERNAL STANDARD	VERIFIED	09:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:48
BLANK TEST	0.00	09:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:49
BLANK TEST	0.00	09:50

26-8449

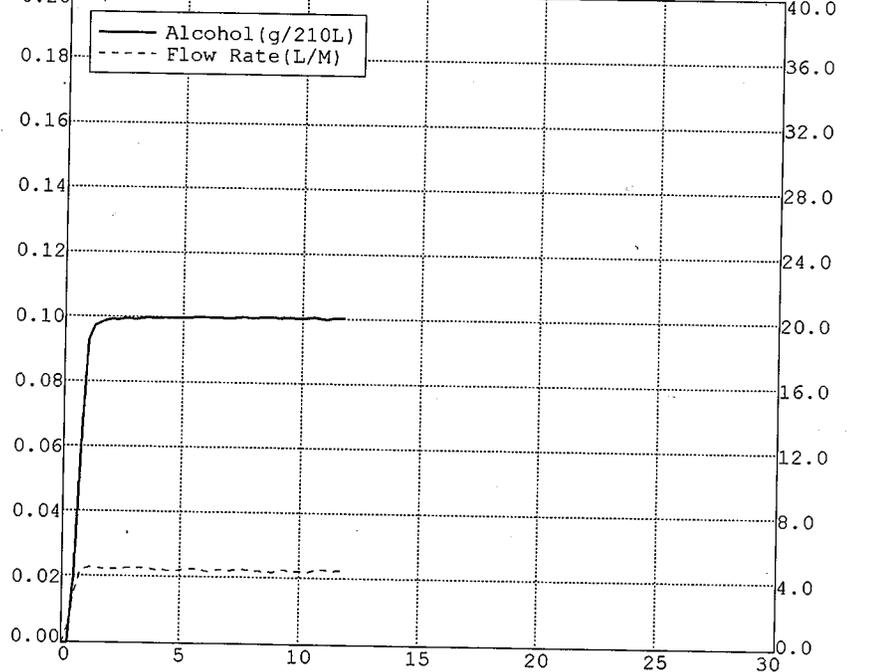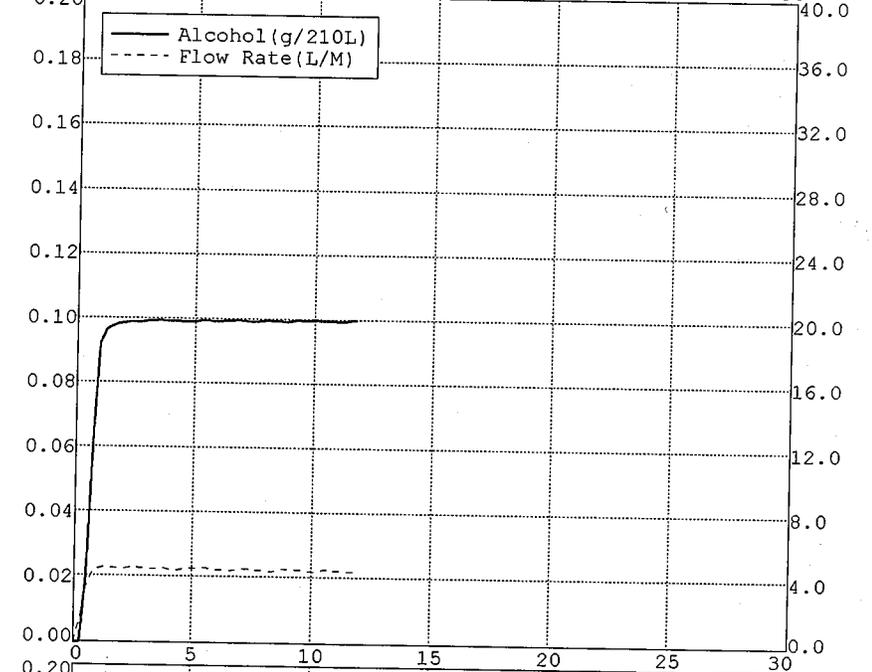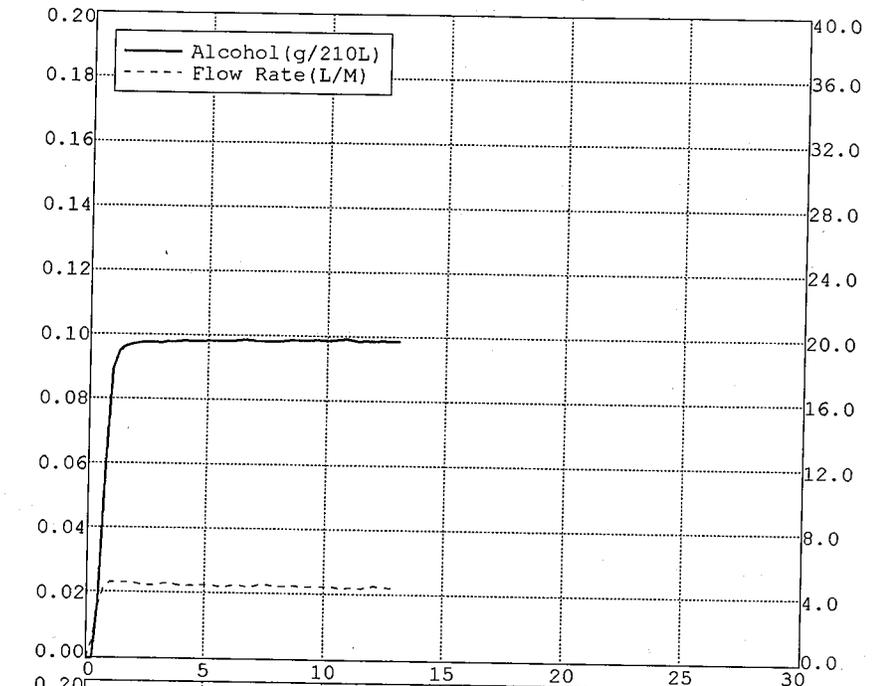

SOLUTION CHANGE

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 03/03/2026

OPERATOR NAME:  
MICHAEL J CLIVE  
Permit #: 36682  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:13
INTERNAL STANDARD	VERIFIED	09:13
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:13
BLANK TEST	0.00	09:14
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:14
BLANK TEST	0.00	09:15
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:15
BLANK TEST	0.00	09:16

26 = 8449

