

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 03/24/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:59
INTERNAL STANDARD	VERIFIED	07:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:00
BLANK TEST	0.00	08:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:01
BLANK TEST	0.00	08:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	08:02
BLANK TEST	0.00	08:03

26-11383

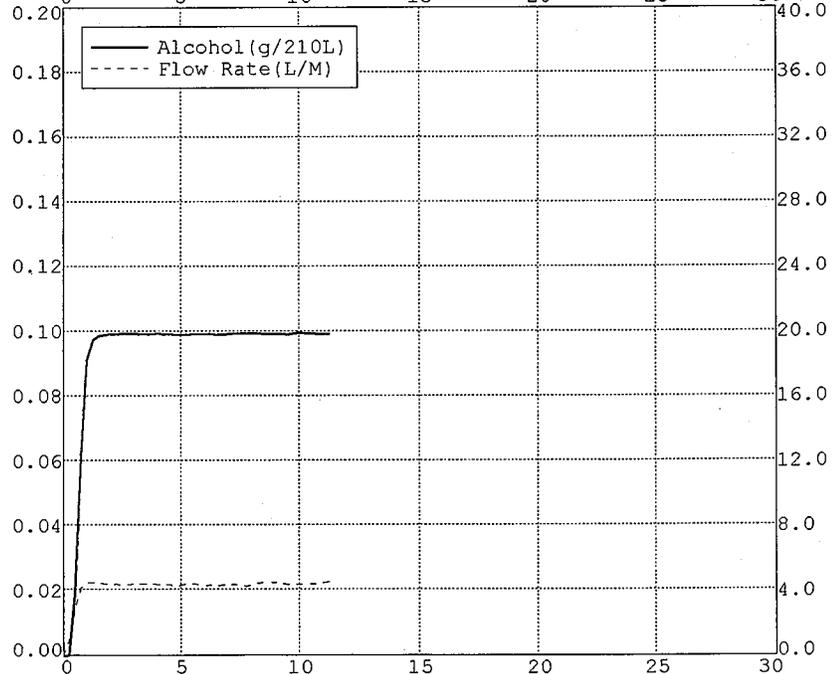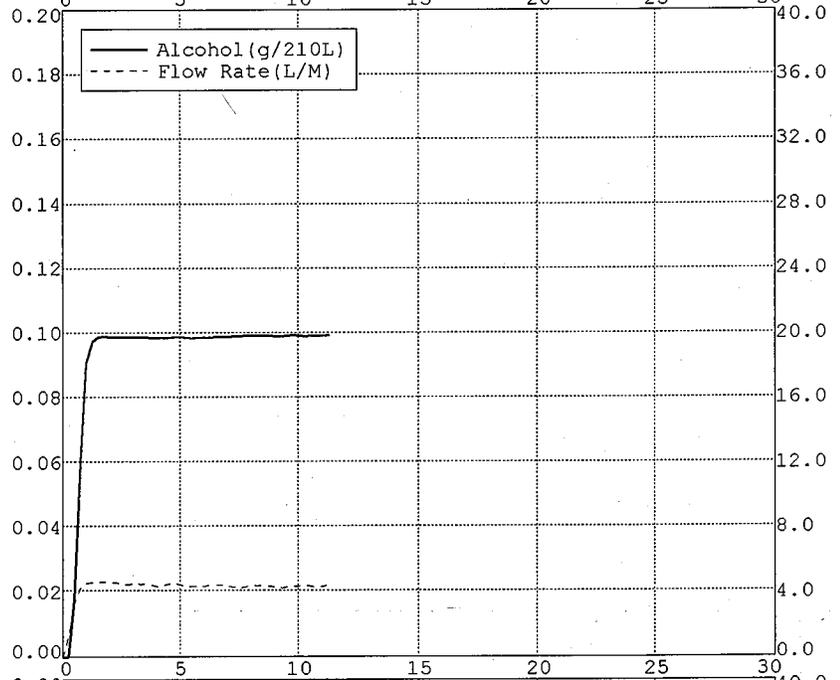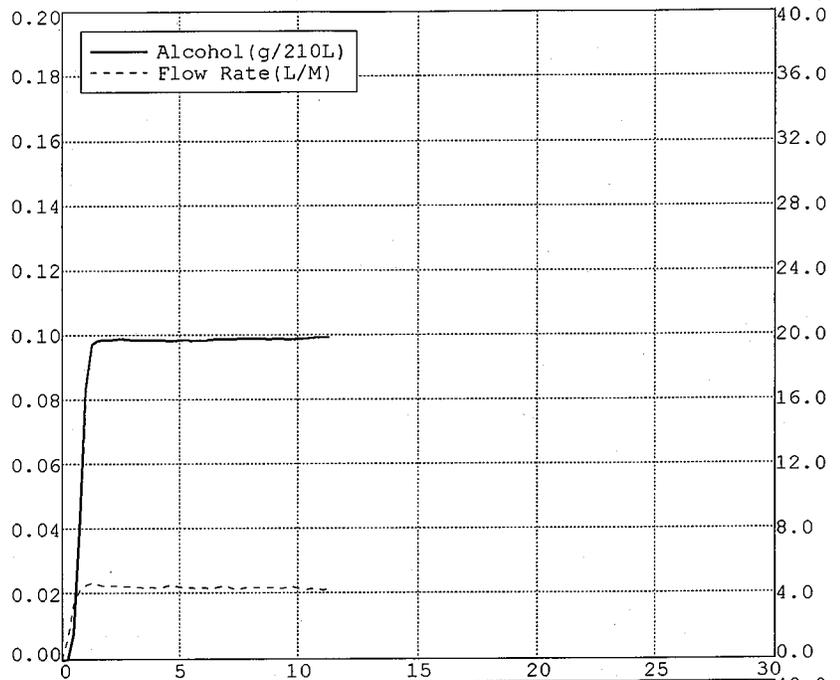

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 03/24/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:56
INTERNAL STANDARD	VERIFIED	07:56
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:56
BLANK TEST	0.00	07:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:57
BLANK TEST	0.00	07:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	07:58
BLANK TEST	0.00	07:59

26-11383

