

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 05/12/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:10
INTERNAL STANDARD	VERIFIED	14:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:10
BLANK TEST	0.00	14:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:11
BLANK TEST	0.00	14:12
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	14:13
BLANK TEST	0.00	14:13

26-18502

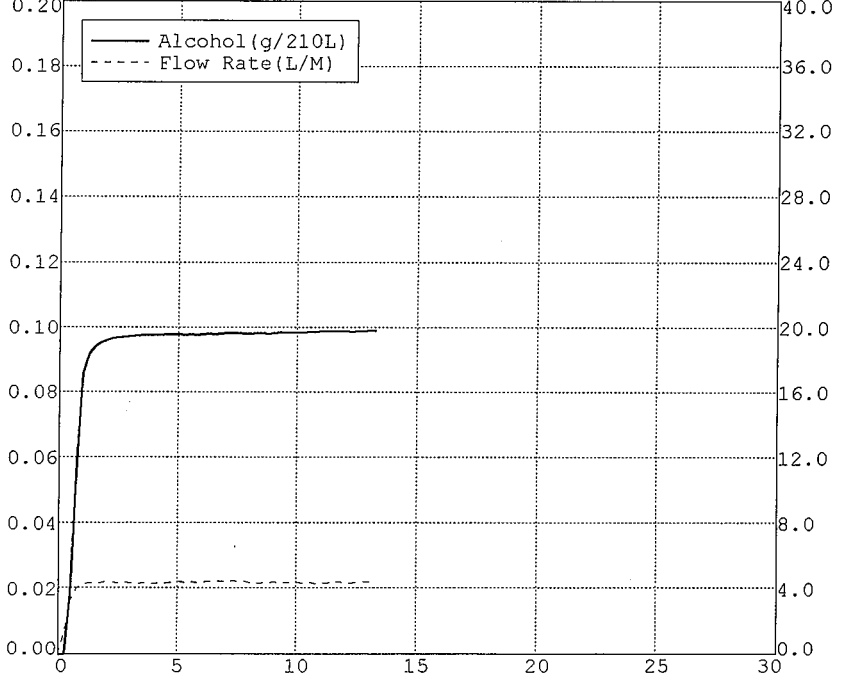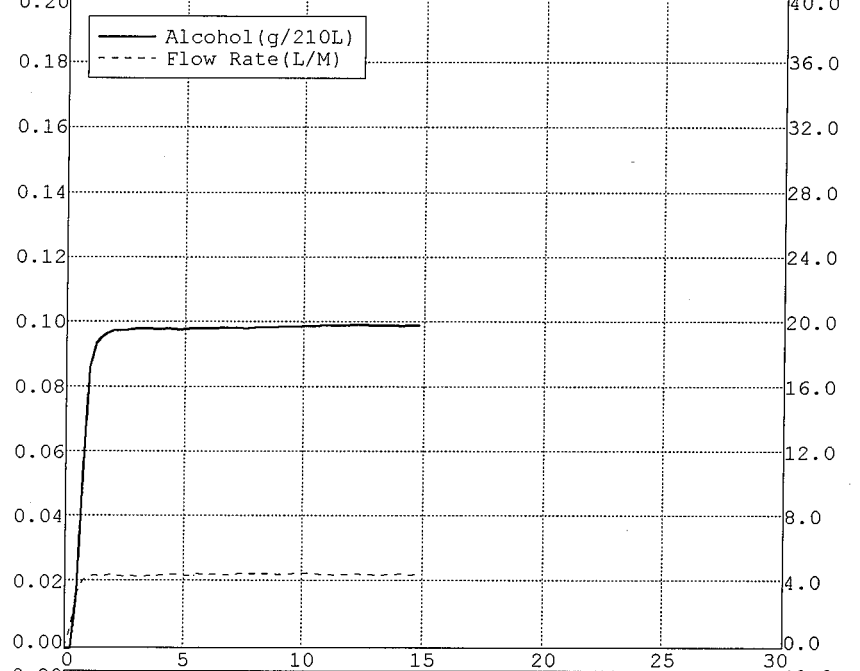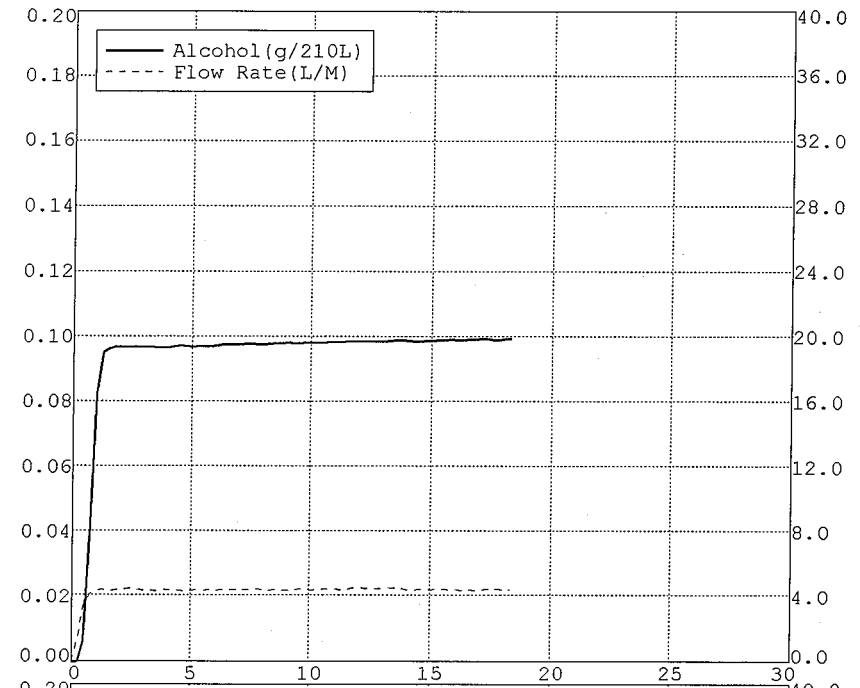

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 05/12/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:10
INTERNAL STANDARD	VERIFIED	14:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:10
BLANK TEST	0.00	14:11
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:11
BLANK TEST	0.00	14:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:12
BLANK TEST	0.00	14:13

26-18502

