

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 107308




Date: 05/19/2026

OPERATOR NAME:  
JOSHUA R HARRINGTON  
Permit #: 38303  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:55
INTERNAL STANDARD	VERIFIED	09:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:56
BLANK TEST	0.00	09:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:57
BLANK TEST	0.00	09:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:58
BLANK TEST	0.00	09:59

26-19322

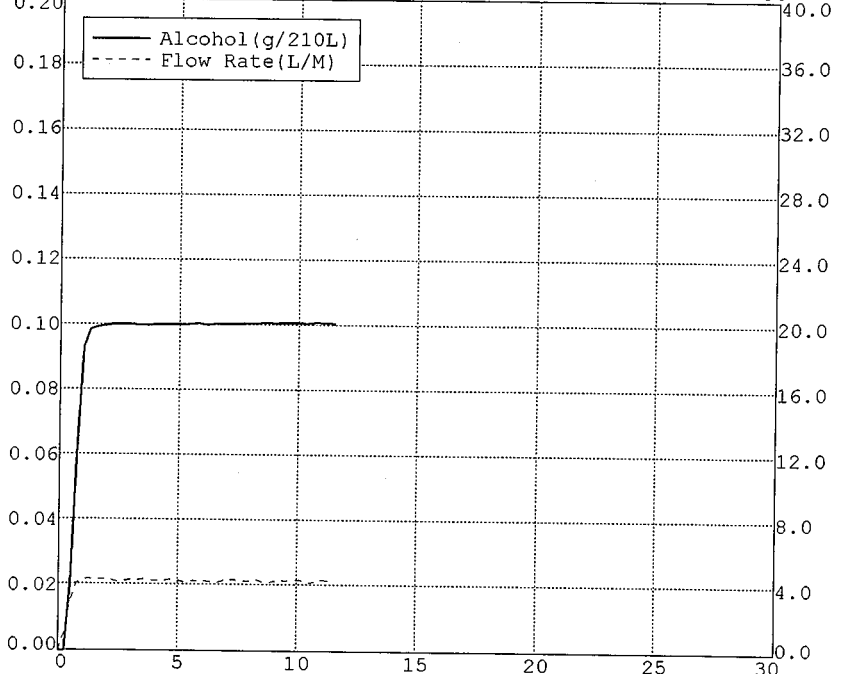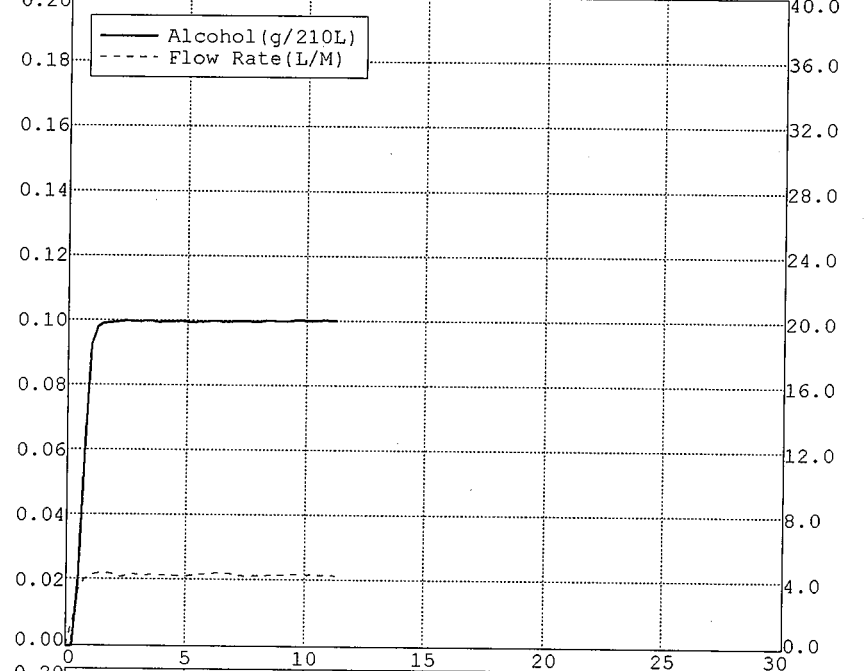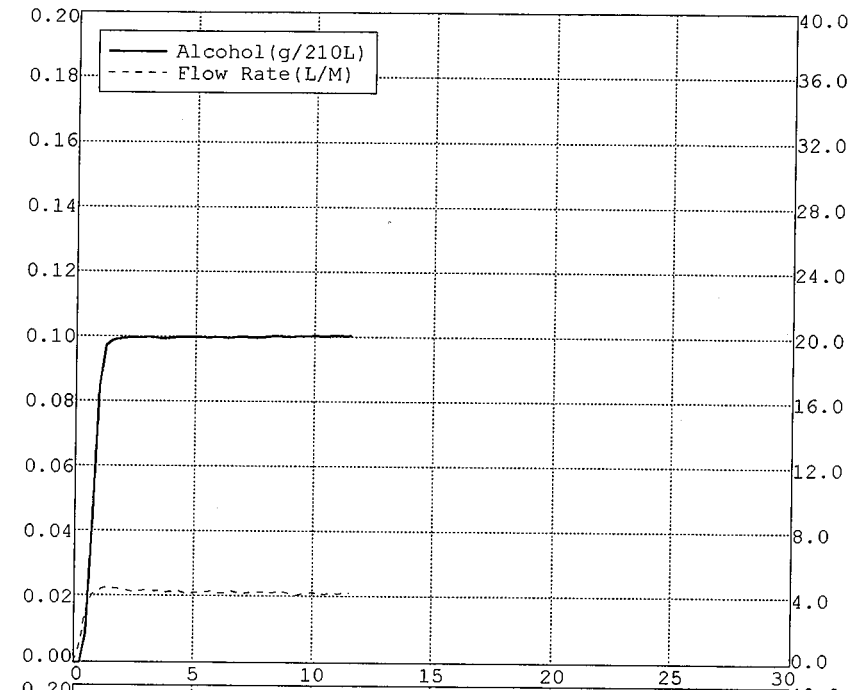

SUPERVISOR TEST

UTICA CITY  
POLICE DEPT  
DATAMASTER dmt: 100282

Date: 05/19/2026

OPERATOR NAME:  
JOSHUA R HARRINGTON  
Permit #: 38303  
Operator Agency/Dept: UTICA CITY PD  
Reference Standard #: 26050

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:55
INTERNAL STANDARD	VERIFIED	09:55
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:56
BLANK TEST	0.00	09:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:57
BLANK TEST	0.00	09:58
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:58
BLANK TEST	0.00	09:59

26-19322

