

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 06/18/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:35
INTERNAL STANDARD	VERIFIED	09:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:36
BLANK TEST	0.00	09:37
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:37
BLANK TEST	0.00	09:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:38
BLANK TEST	0.00	09:39

26-23853

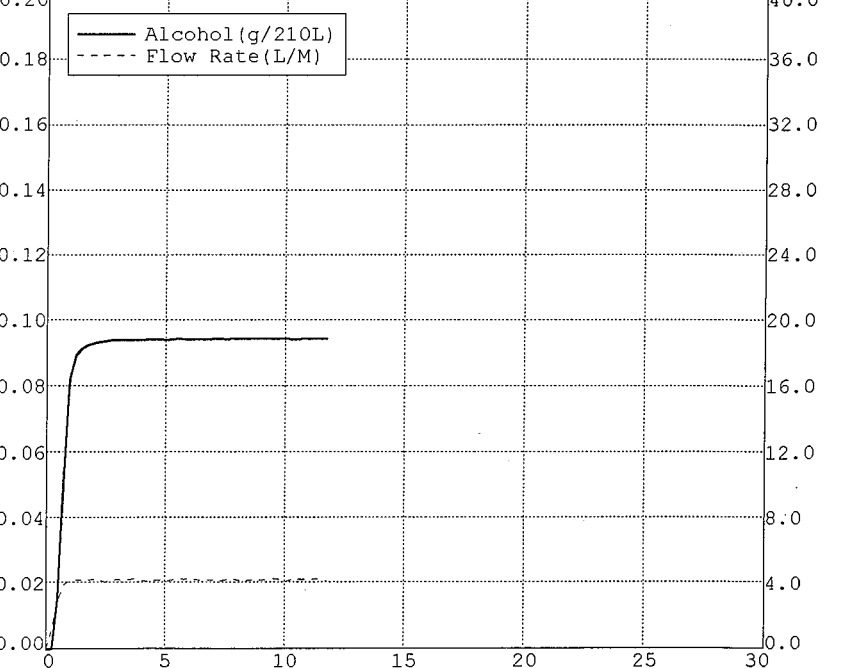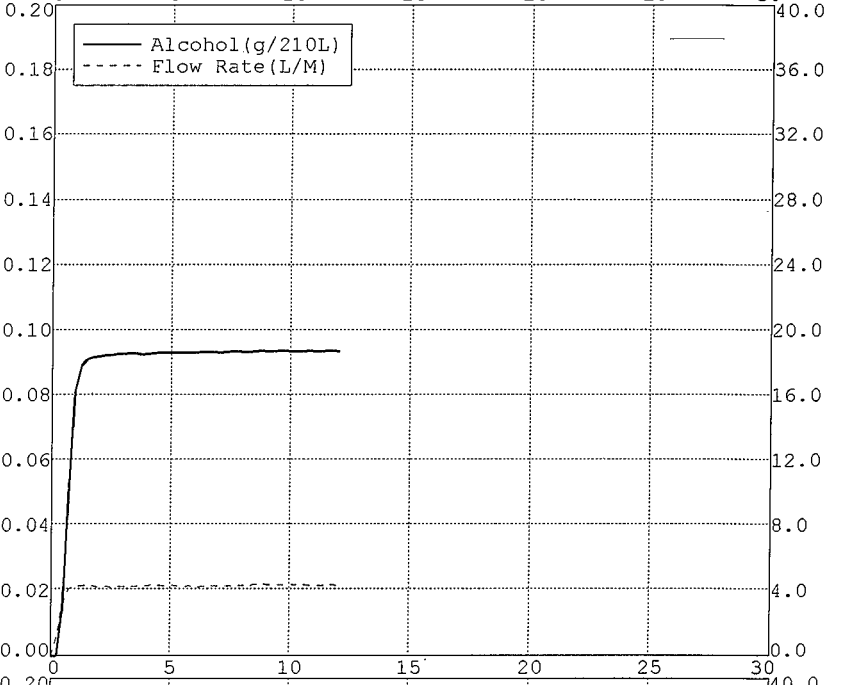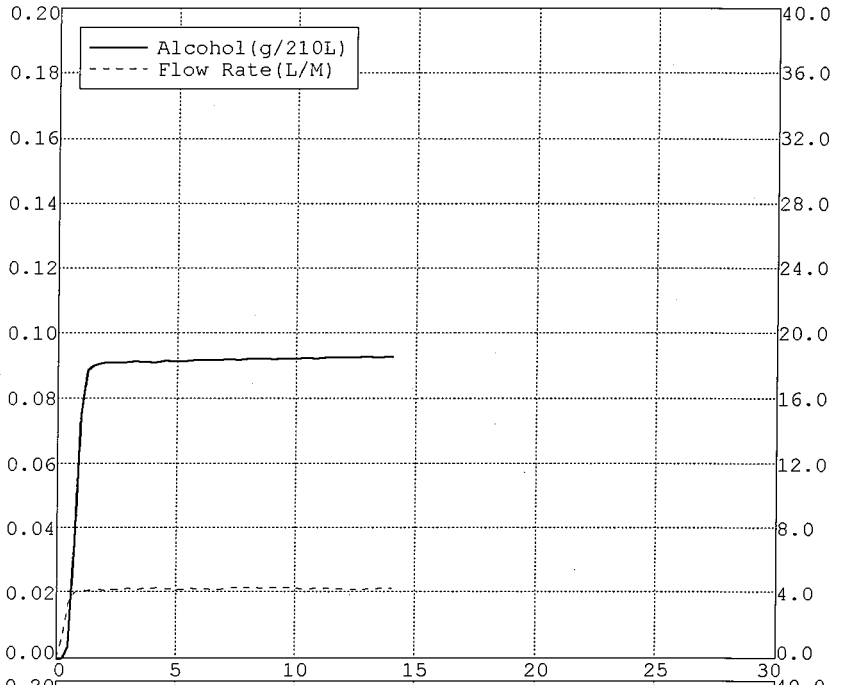

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 06/18/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:42
INTERNAL STANDARD	VERIFIED	09:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:42
BLANK TEST	0.00	09:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:43
BLANK TEST	0.00	09:44
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:44
BLANK TEST	0.00	09:45

26-23853

