

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 07/28/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:32
INTERNAL STANDARD	VERIFIED	09:32
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:33
BLANK TEST	0.00	09:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:34
BLANK TEST	0.00	09:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	09:35
BLANK TEST	0.00	09:36

26-30103

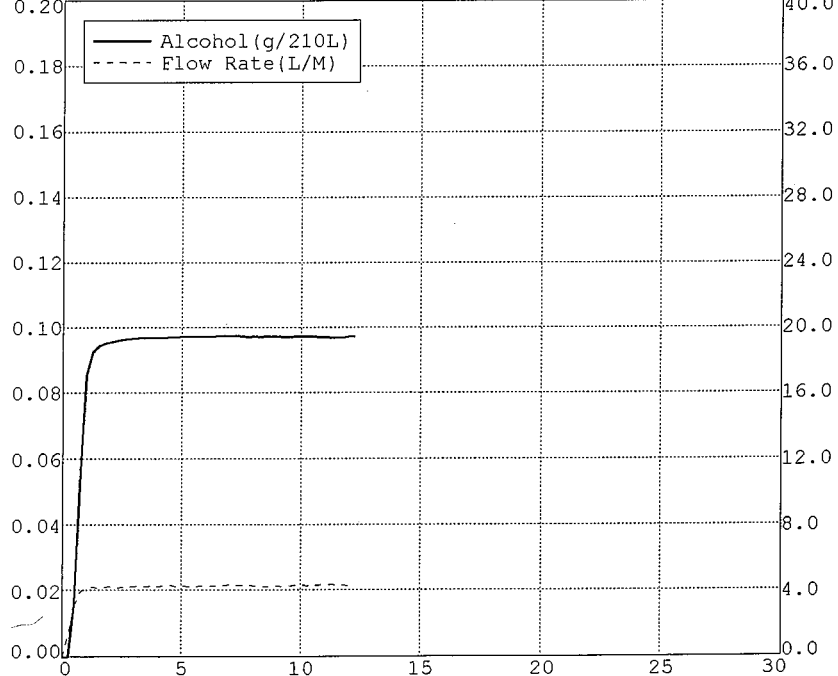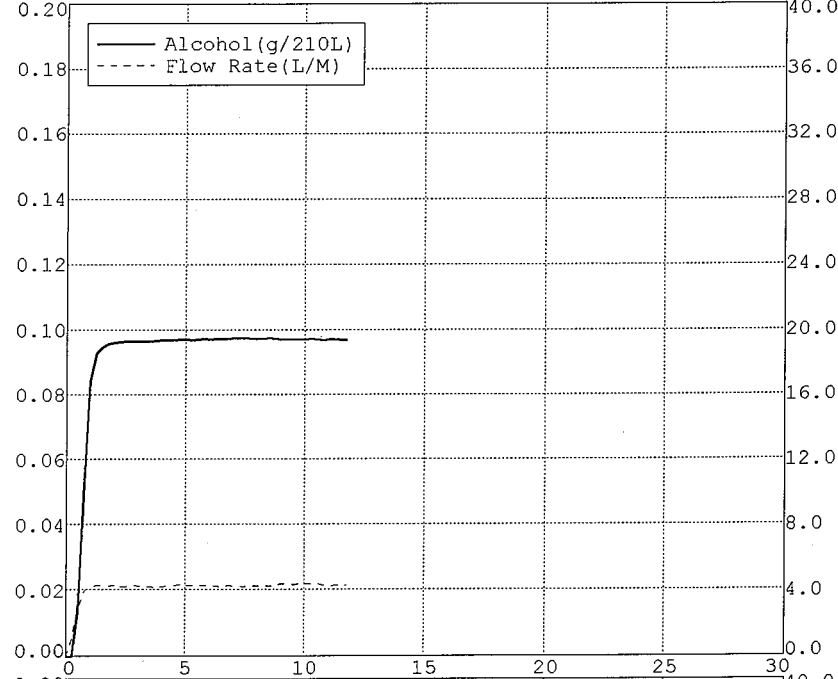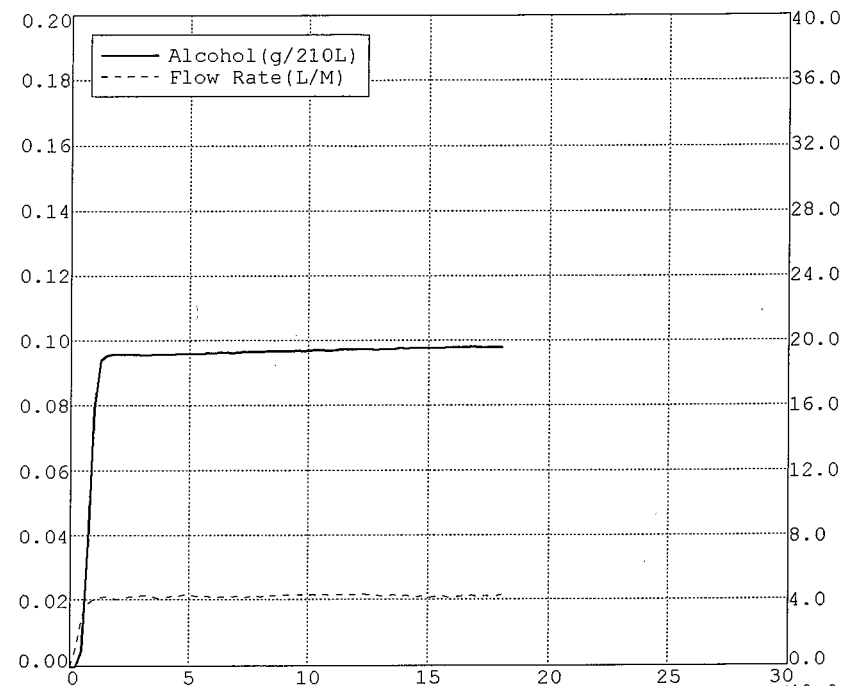

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 07/28/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26120

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:47
INTERNAL STANDARD	VERIFIED	09:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:47
BLANK TEST	0.00	09:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:48
BLANK TEST	0.00	09:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	09:49
BLANK TEST	0.00	09:50

26-30103

