

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282




Date: 08/12/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:38
INTERNAL STANDARD	VERIFIED	10:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:38
BLANK TEST	0.00	10:39
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:40
BLANK TEST	0.00	10:41
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:41
BLANK TEST	0.00	10:42

26-32580

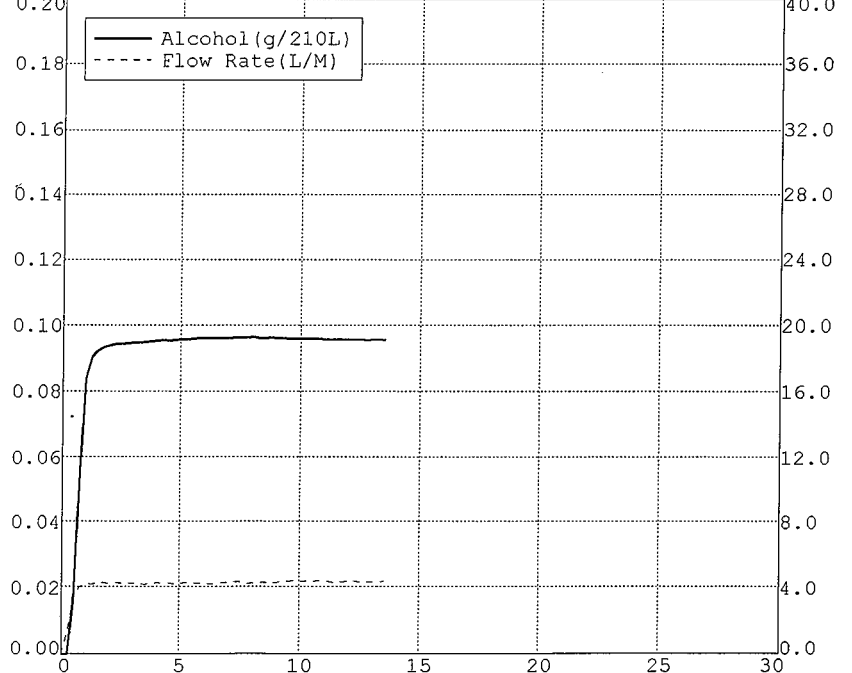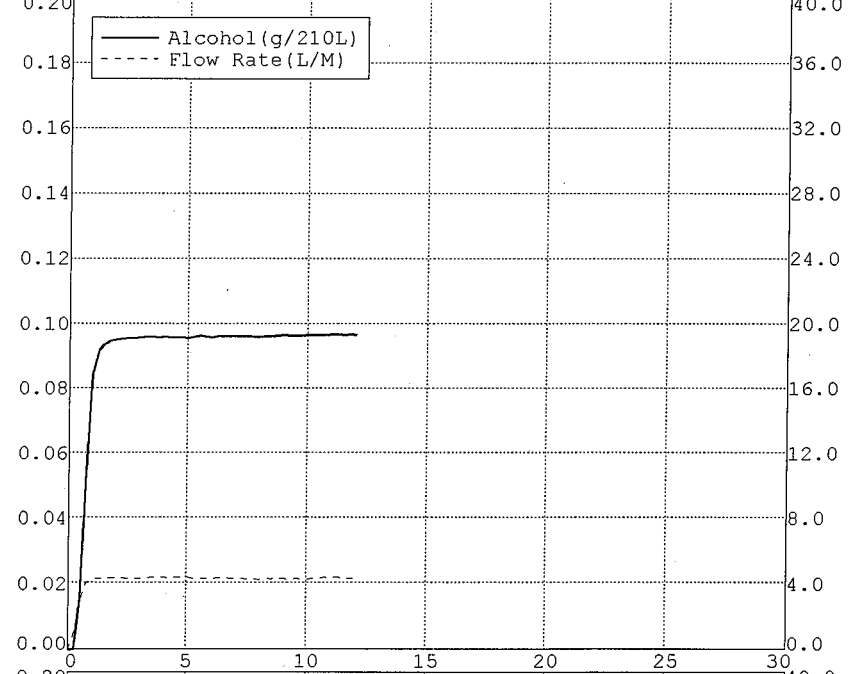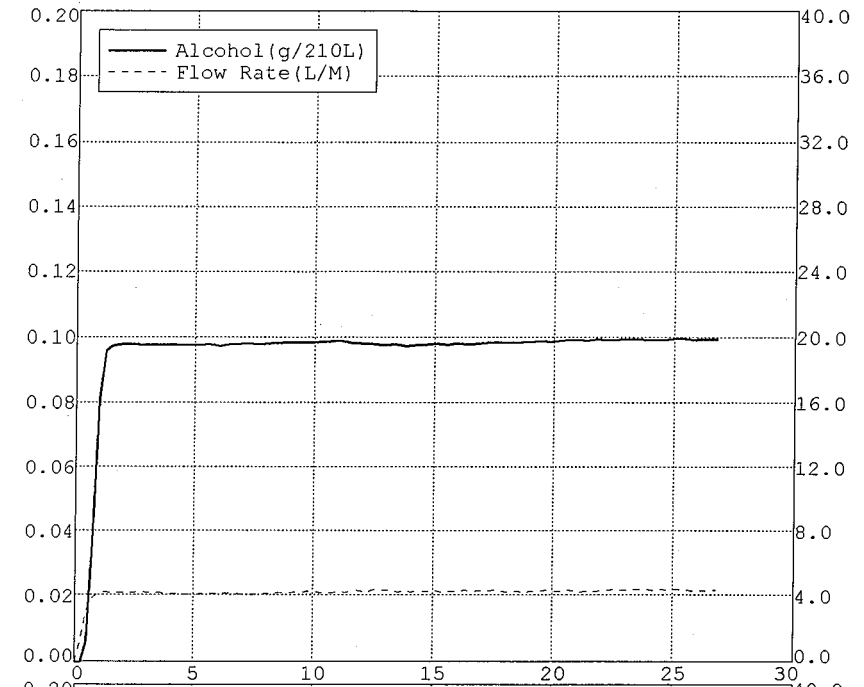

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308

Date: 08/12/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:49
INTERNAL STANDARD	VERIFIED	10:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:49
BLANK TEST	0.00	10:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:50
BLANK TEST	0.00	10:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:51
BLANK TEST	0.00	10:52

26-32580

