SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308


Date: 11/10/2026


OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26270


Nominal = 0.10 g/210L

BLANK TEST	0.00	12:03
INTERNAL STANDARD	VERIFIED	12:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:04
BLANK TEST	0.00	12:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:05
BLANK TEST	0.00	12:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	12:06
BLANK TEST	0.00	12:07

26-45207

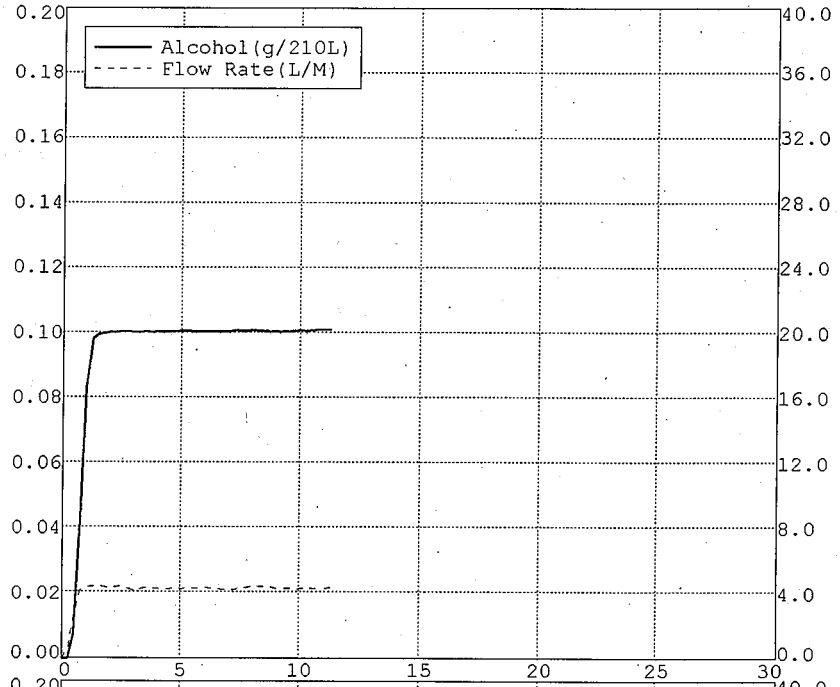

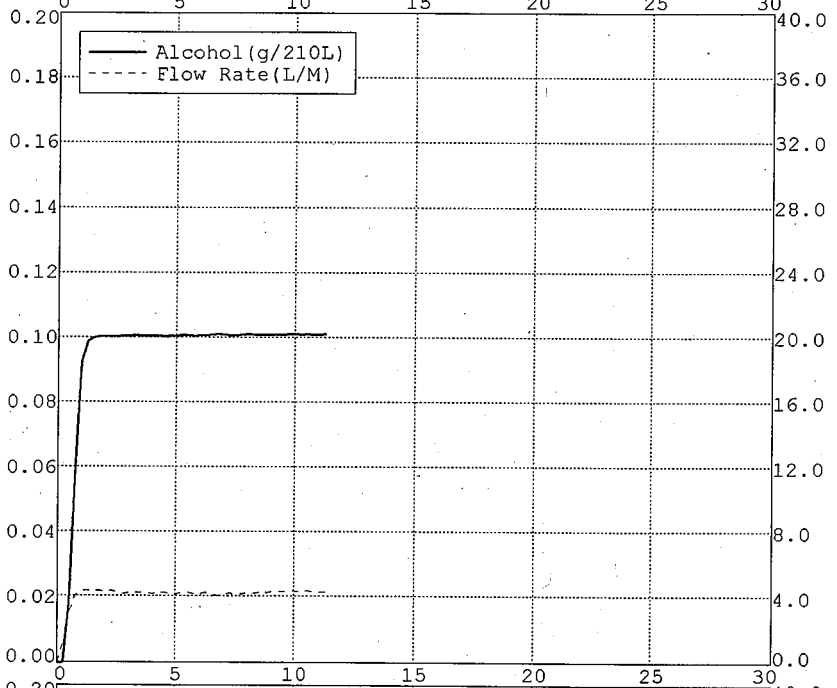

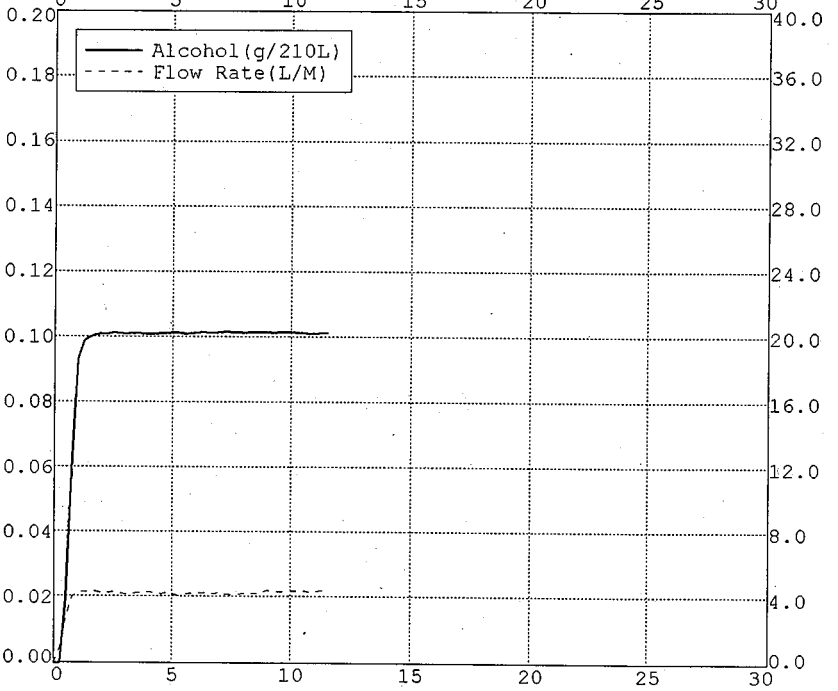

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 11/10/2026

OPERATOR NAME:
JOSHUA R HARRINGTON
Permit #: 38303
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 26270

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:02
INTERNAL STANDARD	VERIFIED	12:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:03
BLANK TEST	0.00	12:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:04
BLANK TEST	0.00	12:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:05
BLANK TEST	0.00	12:06

26-45207

