

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 107308




Date: 02/10/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:38
INTERNAL STANDARD	VERIFIED	10:38
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:38
BLANK TEST	0.00	10:39
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:39
BLANK TEST	0.00	10:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:40
BLANK TEST	0.00	10:41

26-5762

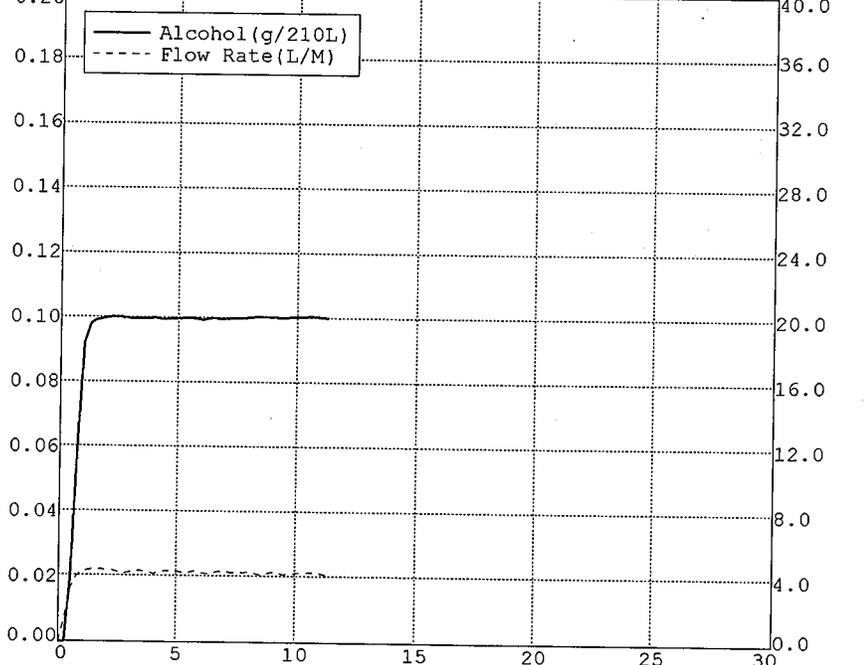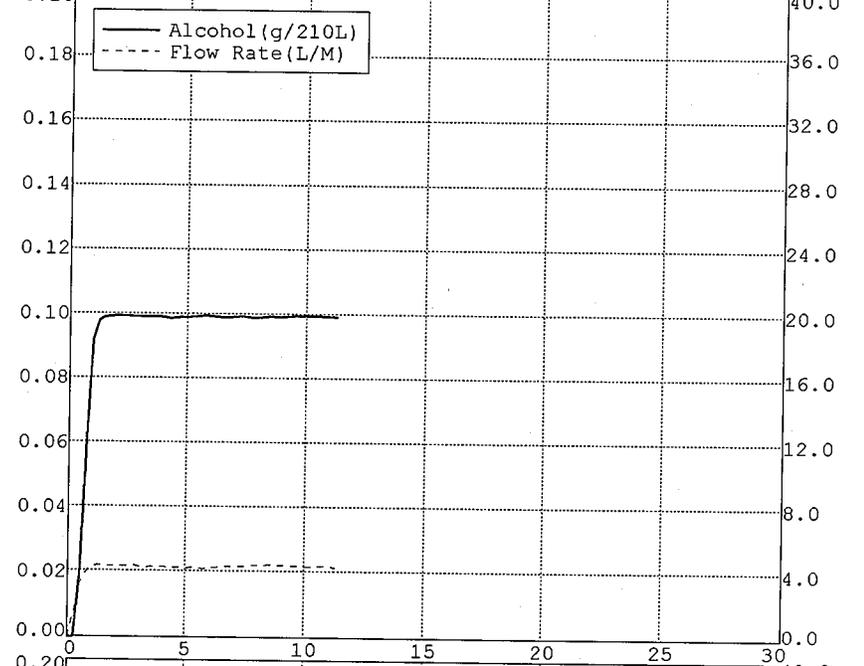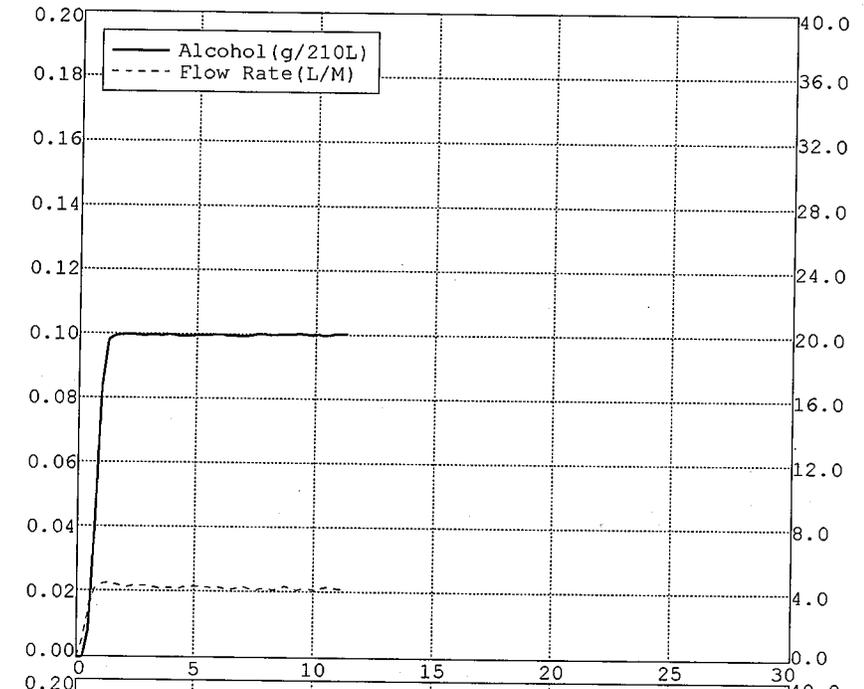

SUPERVISOR TEST

UTICA CITY
POLICE DEPT
DATAMASTER dmt: 100282

Date: 02/10/2026

OPERATOR NAME:
MICHAEL J CLIVE
Permit #: 36682
Operator Agency/Dept: UTICA CITY PD
Reference Standard #: 25390

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:35
INTERNAL STANDARD	VERIFIED	10:35
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	10:38
BLANK TEST	0.00	10:39

26-5762

